



Slimline Elbow EB2040-00

Single Patient Use Only

Rx Only

Important Information

Read carefully and completely before applying.

Intended Use


This elbow brace provides elbow immobilization or range of motion limitations as prescribed by a medical practitioner. It may be used post injury, post-operatively or throughout rehabilitation.

Precautions

Consult your medical professional immediately if you experience sensation changes, unusual reactions, swelling or prolonged pain while using this product.


Directions for Use

1. Remove the elbow brace from package. Remove single hex screw located on brace hinge with hex tool. This will allow clear plastic cover to slide.



Adjust the hinge setting by rotating the clear cover until the desired flexion or extension pins are exposed. Remove the pin from its position and place it in the desired flexion or extension setting. Rotate the clear cover again to cover the flexion and extension pins. Reinsert hex screw using hex tool.


2. Remove foam biceps wrap and forearm wrap from inside of brace.




3. Position the biceps and forearm wraps on patient so that the hook-and-loop closure is located

on the anterior (front) surface of the arm. Trim excess material to allow approximately 2" overlap.

4. Position the brace so that the hinges are aligned with the center of the elbow joints of the arm.



5. With the hinge settings aligned properly, begin attaching the hook-and-loop closure straps. First attach the strap directly above the elbow. Next attach the strap just below the elbow. Finally attach the strap closest to the shoulder followed by the strap closest to the hand.




Manufacturer

DeRoyal
200 DeBusk Lane, Powell, TN 37849 U.S.A.
888.938.7828
865.938.7828

Authorized Representative

DeRoyal Europe, Ltd.
Virginia Road, Kells, County Meath Ireland
353.46.9280100

©2004 DeRoyal. All Rights Reserved.
Part #0-847 Revision A
Revised 2/04

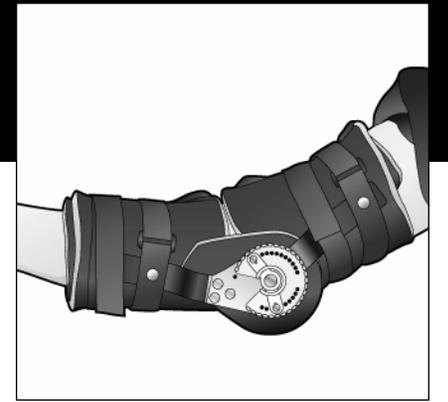

Slimline Elbow EB2040-00

Single Patient Use Only

Rx Only

Important Information

Read carefully and completely before applying.

Intended Use


This elbow brace provides elbow immobilization or range of motion limitations as prescribed by a medical practitioner. It may be used post injury, post-operatively or throughout rehabilitation.

Precautions

Consult your medical professional immediately if you experience sensation changes, unusual reactions, swelling or prolonged pain while using this product.


Directions for Use

1. Remove the elbow brace from package. Remove single hex screw located on brace hinge with hex tool. This will allow clear plastic cover to slide.



Adjust the hinge setting by rotating the clear cover until the desired flexion or extension pins are exposed. Remove the pin from its position and place it in the desired flexion or extension setting. Rotate the clear cover again to cover the flexion and extension pins. Reinsert hex screw using hex tool.


2. Remove foam biceps wrap and forearm wrap from inside of brace.




3. Position the biceps and forearm wraps on patient so that the hook-and-loop closure is located

on the anterior (front) surface of the arm. Trim excess material to allow approximately 2" overlap.

4. Position the brace so that the hinges are aligned with the center of the elbow joints of the arm.



5. With the hinge settings aligned properly, begin attaching the hook-and-loop closure straps. First attach the strap directly above the elbow. Next attach the strap just below the elbow. Finally attach the strap closest to the shoulder followed by the strap closest to the hand.




Manufacturer

DeRoyal
200 DeBusk Lane, Powell, TN 37849 U.S.A.
888.938.7828
865.938.7828

Authorized Representative

DeRoyal Europe, Ltd.
Virginia Road, Kells, County Meath Ireland
353.46.9280100

©2004 DeRoyal. All Rights Reserved.
Part #0-847 Revision A
Revised 2/04

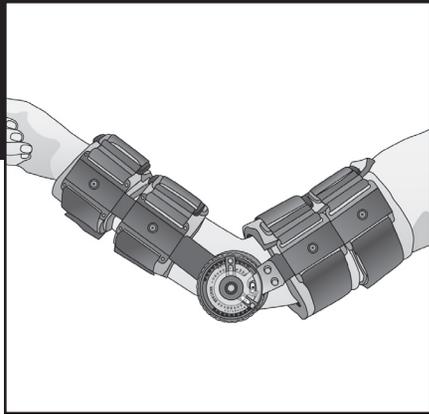

Transition Elbow Brace

Single Patient Use Only

Rx Only

IMPORTANT INFORMATION

Please read all instructions, warnings, and precautions before use.

INTENDED USE

This brace provides elbow immobilization or range of motion limitations as prescribed by a clinician. It may be used post injury, post-operatively or throughout rehabilitation.

PRECAUTIONS

Consult your clinician immediately if you experience sensation changes, unusual reactions, swelling or increased pain while using this product. Use caution when fitting this product on patients with reduced sensitivity. Patients with circulation problems should use caution when tightening the straps. Product should be worn during activity only. Remove product when in a resting position or sleeping.








SIZING

Measure from the axis of the elbow to the axis of the wrist.

Small	6" – 8"
Medium	8" – 10"
Large	10" or more

INSTRUCTIONS FOR USE

1. To adjust hinge setting, rotate clear face cover to the desired flexion or extension control points.
2. Pull the control pin carriers straight away from the hinge.
3. Rotate control pin carriers to the desired settings.
4. Reseat the control pin carriers in the desired setting points.
5. Rotate the clear face cover to reset it in its original position.
6. Repeat this procedure on the opposite side of the brace.
7. Remove forearm and biceps foam wraps from elbow hinges.
8. Position the forearm and biceps foam wraps so the hook and loop closures are located on the anterior (front) surface of the arm. Trim excess material to allow approximately 2" overlap.

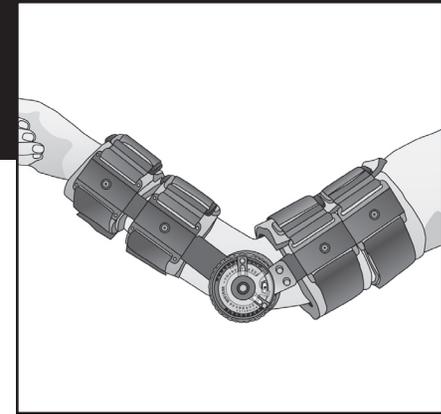

Transition Elbow Brace

Single Patient Use Only

Rx Only

IMPORTANT INFORMATION

Please read all instructions, warnings, and precautions before use.

INTENDED USE

This brace provides elbow immobilization or range of motion limitations as prescribed by a clinician. It may be used post injury, post-operatively or throughout rehabilitation.

PRECAUTIONS

Consult your clinician immediately if you experience sensation changes, unusual reactions, swelling or increased pain while using this product. Use caution when fitting this product on patients with reduced sensitivity. Patients with circulation problems should use caution when tightening the straps. Product should be worn during activity only. Remove product when in a resting position or sleeping.








SIZING

Measure from the axis of the elbow to the axis of the wrist.

Small	6" – 8"
Medium	8" – 10"
Large	10" or more


INSTRUCTIONS FOR USE

1. To adjust hinge setting, rotate clear face cover to the desired flexion or extension control points.
2. Pull the control pin carriers straight away from the hinge.
3. Rotate control pin carriers to the desired settings.
4. Reseat the control pin carriers in the desired setting points.
5. Rotate the clear face cover to reset it in its original position.
6. Repeat this procedure on the opposite side of the brace.
7. Remove forearm and biceps foam wraps from elbow hinges.
8. Position the forearm and biceps foam wraps so the hook and loop closures are located on the anterior (front) surface of the arm. Trim excess material to allow approximately 2" overlap.







9. Position the brace so the hinges are aligned with the center of the elbow joint on either side of the arm. Determine if length of the brace's arms need to be adjusted.




10. To adjust length of the arms of the brace, loosen screw at distal (farthest) end of brace with hex tool and slide attachment. Break off excess metal at indentation on brace by applying force (i.e. breaking on the end of a table).



Repeat on opposite arm. Retighten screws after adjustment. **NOTE: DO NOT OVERTIGHTEN SCREWS.**

11. When adjusted, align hinges with the center of the elbow joint on either side of the arm. Secure hinges to foam wraps with hook closures on inside of brace arms and hinge.



12. Secure with loop lock closure straps.

WASHING INSTRUCTIONS

Hand wash foam wraps in cool water with mild detergent. Air dry.




Distributed by DeRoyal
200 DeBusk Lane
Powell, TN 37849 U.S.A.
888.938.7828
865.938.7828

Manufactured by Vantage Orthopedics, Inc
41 Techview Drive
Cincinnati, OH 45215



Part #0-1820
©2005 DeRoyal. All Rights Reserved.
Revised 7/05



9. Position the brace so the hinges are aligned with the center of the elbow joint on either side of the arm. Determine if length of the brace's arms need to be adjusted.




10. To adjust length of the arms of the brace, loosen screw at distal (farthest) end of brace with hex tool and slide attachment. Break off excess metal at indentation on brace by applying force (i.e. breaking on the end of a table).



Repeat on opposite arm. Retighten screws after adjustment. **NOTE: DO NOT OVERTIGHTEN SCREWS.**

11. When adjusted, align hinges with the center of the elbow joint on either side of the arm. Secure hinges to foam wraps with hook closures on inside of brace arms and hinge.



12. Secure with loop lock closure straps.

WASHING INSTRUCTIONS

Hand wash foam wraps in cool water with mild detergent. Air dry.



Distributed by DeRoyal
200 DeBusk Lane
Powell, TN 37849 U.S.A.
888.938.7828
865.938.7828

Manufactured by Vantage Orthopedics, Inc
41 Techview Drive
Cincinnati, OH 45215

Part #0-1820
©2005 DeRoyal. All Rights Reserved.
Revised 7/05